



OPEN ACCESS

Use of the GeneReader NGS System in a clinical pathology laboratory: a comparative study

Ulrike Koitzsch,¹ Carina Heydt,¹ Hans Attig,² Isabelle Immerschitt,¹ Sabine Merkelbach-Bruse,¹ Alessandro Fammartino,² Reinhard H Büttner,^{1,3} Yi Kong,¹ Margarete Odenthal^{1,3}

► Additional material is published online only. To view please visit the journal online (<http://dx.doi.org/10.1136/jclinpath-2017-204342>).

¹Institute of Pathology, University Hospital of Cologne, Cologne, Germany

²QIAGEN GmbH, Hilden, Germany

³Center of Molecular Medicine Cologne (CMMC), University of Cologne, Cologne, Germany

Correspondence to

Dr Margarete Odenthal, Institute of Pathology, University Hospital of Cologne, Kerpener Str. 62, Koeln 50924, Germany; m.odenthal@uni-koeln.de

UK and CH contributed equally.

Received 11 January 2017

Revised 27 February 2017

Accepted 28 February 2017

Published Online First

11 April 2017

ABSTRACT

Despite its successful use in academic research, next-generation sequencing (NGS) still represents many challenges for routine clinical adoption due to its inherent complexity and specialised expertise typically required to set-up, test and operate a complete workflow. This study aims to evaluate QIAGEN's newly launched GeneReader NGS System solution in a pathology laboratory setting by assessing the system's ease of use, sequencing accuracy and data reproducibility. Our laboratory was able to implement the system and validate its performance using clinical samples in direct comparison to an approved Sanger sequencing platform and to an alternative in-house NGS technology. The QIAGEN workflow focuses on clinically actionable hotspots maximising testing efficiency. Combined with automated upstream sample processing and integrated downstream bioinformatics, it offers a realistic solution for pathology laboratories with limited prior experience in NGS technology.

INTRODUCTION

Next-generation sequencing (NGS) holds the potential to transform our understanding, treatment and management of cancer. Not only does it offer unprecedented genetic insights at a molecular level, it also enables personalised cancer treatment to maximise effectiveness. Targeted application of NGS technology allows the identification of specific mutations that affect cancer evolution and its likely response to a particular regimen, thus providing an essential tool in guiding clinical decisions.¹ As such, oncologists are increasingly requesting molecular testing of cancer samples. In addition, in a clinical pathology laboratory, targeted NGS has the advantages of low sample input,^{1,2} high volume throughput and the ability to simultaneously interrogate multiple genes.³ For biopsy-based cancer diagnosis, where the tissue source is often limited, the ability to gain maximum insights from minimal sample material is particularly beneficial.² As such, many pathology laboratories such as ours are faced with a pressing need to establish an NGS workflow to meet these requirements.

However, a number of challenges still exist against widespread adoption of NGS in clinical diagnostics laboratories. These include substantial equipment and operational costs, often complex workflows and the need for specialised bioinformatics capabilities to analyse and interpret the data for clinically meaningful use. To this end, QIAGEN recently launched the GeneReader NGS System

offering a complete solution with a reduced hands-on time and fully integrated bioinformatics pipeline. This system is aimed at removing these barriers and enabling more laboratory to use the NGS technology.

To test the performance of the system, we conducted a comparison study between the GeneReader and an alternative in-house NGS platform. We tested formalin-fixed and paraffin-embedded (FFPE) clinical tumour samples taken from a range of cancer types (colorectal and gastric carcinoma, lung cancer, melanoma and gastrointestinal stromal tumours (GIST)) and processed them in two parallel workflows. Mutational status and variant allele frequencies were compared and verified via Sanger sequencing. Here we report highly consistent results from both workflows. Furthermore, we assessed the usability of the GeneReader System in a clinical pathology laboratory setting. Our experience confirms that the GeneReader NGS System is suitable for routine pathology laboratory use.

MATERIALS AND METHODS

Sample and DNA isolation

FFPE tumour material from various clinical sources has been collected at the Institute for Pathology at the University Hospital of Cologne. The following tumour tissue types have been considered: colorectal cancer (CRC), lung cancer, melanoma, GIST and gastric cancer (table 1). All samples were processed by the routine diagnostic pipeline of the Institute for Pathology in the years 2015 and 2016. The genomic DNA (gDNA) extracts, all characterised for the tumour/normal cells ratio and for clinical relevant mutations by the in-house NGS pipeline, based on the Illumina MiSeq, were selected as listed in table 1 for our study.

Tumorous areas were marked by senior pathologists, and tumour nodules were scraped off from 3 to 9 µm thick sections corresponding to the H&E stained section. Automated DNA isolation from the macrodissected tumour areas has been then carried out using the Maxwell 16 FFPE Tissue low-elution volume DNA Purification Kit on a Maxwell 16 instrument (Promega GmbH, Mannheim, Germany) as described previously.^{4,5,6} To determine PCR accessible DNA, real-time quantitative PCR (qPCR) was performed using a standard curve of high-quality human gDNA (Takara/Clontech, Saint-Germain-en-Laye, France) ranging from 0.195 to 50 ng. qPCR targeting a 234 bp region of the *HFE* gene was then carried out in duplicates



CrossMark

To cite: Koitzsch U, Heydt C, Attig H, et al. *J Clin Pathol* 2017;**70**:725–728.

Short report

Table 1 Clinical samples considered by this study with indication of the tumour percentage present in the relative formalin-fixed and paraffin-embedded material and in the targeted genes

Cancer type	Sample number	Tumour, %	Hot spot mutations
CRC*	15	30%–90%; mean=40%	KRAS, NRAS, BRAF, PIK3CA
Lung (NSCLC)	16	20%–70%; mean=30%	KRAS, EGFR, ERBB2, PIK3CA
Melanoma	8	30%–90%; mean=40%	BRAF, PIK3CA
GIST	8	60%–90%; mean=85%	KIT, PDGFRA
Gastric carcinoma	3	60%; 70%	PIK3CA, KRAS

CRC, colorectal cancer; GIST, gastrointestinal stromal tumour; NSCLC, non-small cell lung cancer.

with 1 μ L DNA, each added to a 20 μ L reaction mix containing GoTaq qPCR Master Mix (Promega) and 0.4 μ M of the HFE forward (TTC TCA GCT CCT GGC TCT CAT C) and reverse primer (TCG AAC CTA AAG ACG TAT TGC CC).^{6 7} The variety of different ages and origin of the FFPE samples used for this study generated different amounts of extracted DNA, as determined by qPCR (see online supplementary table S2). All 50 samples extracted passed qPCR quality control and yielded enough material for further processing. For the target enrichment step, a fixed PCR protocol with 23 or 26 cycles has been used for all samples for the MiSeq and GeneReader workflows, respectively, according to manufacturer's protocol.

GeneReader assay and sequencing

In total, 40 ng of each gDNA was used as template for the QIAGEN Actionable Insight Tumour Panel. The QIAGEN ATP assay amplifies 330 amplicons covering 16.7 kb, interrogating 773 unique variant positions in 12 genes of high prognostic and therapeutic relevance (*KRAS*, *NRAS*, *KIT*, *BRAF*, *PDGFRA*, *ALK*, *EGFR*, *ERBB2*, *PIK3CA*, *ERBB3*, *ESR1* and *RAF1*) (see table 2). Targeted amplicons have been further processed to generate a library for sequencing. Libraries were prepared using the QIAGEN GeneRead DNA Library Kit and an automated

Table 2 Parameter and sequencing coverage results achieved in this study by the Actionable Insight Tumour Panel

Parameter	Details	
Panel size	12 genes/16.7 kb	
Insight size	773 unique variant positions	
Amplicons	330	
Variant allele fraction detection limit	ATPf: 5%; ATPp: 1%	
Frequency cut-off and amplicon coverage	Expected	Measured
	$\geq 500\times$: 90%	Median: 95.41%
	$\geq 200\times$: 95%	Average: 91.71%
Coverage of clinical variants investigated	$\geq 200\times$: 95%	Median: 98.58%
		Average: 97.12%
	Median: 5001 \times	
	Average: 7656 \times	

Positive samples included into the study have all been confirmed by at least one alternative technology: that is, Illumina MiSeq and/or Sanger sequencing technologies. ATPf and ATPp indicate data analysis for the Actionable Tumour Panel assays using different filtering thresholds depending if FFPE (f) or plasma samples (p) are applied. FFPE, formalin fixed and paraffin embedded.

protocol on a QIAcube according to the manufacturer's instructions. Both PCR-enriched DNA and GeneRead libraries were qualified and quantified using a QIAGEN QIAxcel Advanced System according to the manufacturer's instructions. The emulsion PCR and bead enrichment steps were carried out using the GeneRead Clonal Amp Q Kit and an automated protocol on a GeneRead QIAcube according to the manufacturer's instructions. Following clonal amplification, amplicon libraries were sequenced using the QIAGEN GeneRead Sequencing Q Kit and an automated protocol on a GeneReader instrument (all protocols available on <http://www.qiagen.com>).

GeneReader data processing

QIAGEN Clinical Insight Analyze (QCI-A) software performed the secondary analysis of FASTQ reads generated by the GeneReader consisting of alignment of reads to the hg19 reference, calling the variants, generating an interactive report for visualisation and quality control of the sequencing results as well as a summary of the data. All comparable variants have been identified by QCI-A secondary analysis pipeline for the ATP on FFPE material (ATPp), where a 5% allelic fraction cut-off is used to call variants for FFPE samples. In one case, sample Q11, in order to detect a PIK3CA variant (p.E542K) at low allele frequency (2.8%), we had to use the newly launched pipeline for liquid biopsies (ATPp), which allows a 0.5% allelic fraction cut-off.

After reviewing their data validity, variants were imported as industry standard variant call format into the QCI-interpret (QCI-I) web interface, which enables data interpretation for the previously identified variants. QCI-I then generated a per sample report for each detected variant based on the curated content of QIAGEN Knowledge Base including: summary of findings, direct link to the data source and the eventual treatment(s) recommended.

Other material and methods

Reference library construction, Illumina MiSeq sequencing and data analysis as well as Sanger sequencing are described in online supplementary material and methods.

RESULTS AND DISCUSSION

The focus of this study was to conduct a performance validation of the QIAGEN GeneReader NGS System and assess its suitability for routine use in a clinical diagnostic laboratory.

GeneReader sequencing

The laboratory set-up of the in-house established NGS workflow compared with the QIAGEN sample-to-insight NGS solution is shown in the figure 1A. Both workflows take 5 days until the diagnosis can be made. In our in-house pipeline, protocols and reagents used in the different steps of the pipeline have to be synchronised and harmoniously aligned. Therefore, our in-house solution describes a typical case scenario of a pathology laboratory where the full set-up requires prior knowledge to identify relevant kits from different vendors on one hand, but also enables high flexibility on the other hand (figure 1). The GeneReader NGS System clearly showed a close bundle of the different components in a unique product. Furthermore, the high extent of automation and integrated solutions of the GeneReader system resulted in an equal turnaround time, but in a very low hands-on time (<10 hours) (figure 1A, B).


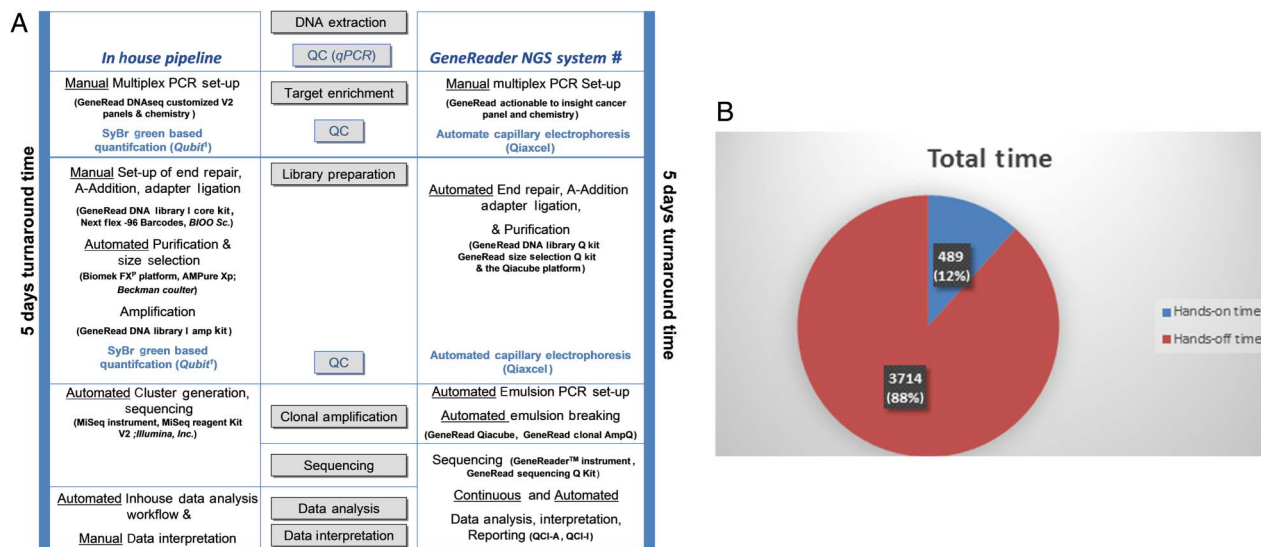


Figure 1 Time course of the in-house pipeline and the GeneReader next-generation sequencing (NGS) System workflow. (A) Both workflows take a turnaround time of 5 days, but numerous automated steps reduce the hands-on time in the GeneReader NGS workflow as shown in B. #Platform and reagents were purchased from Qiagen (Hilden, Germany). ¹Fluorometric quantification by the Qubit instrument and reagents (ThermoFisher Scientific, Darmstadt, Germany). (B) Cake diagram of the turnaround time using the GeneReader NGS System workflow demonstrates a low hands-on time of around 8 hours 15 min (489 min), but a hands-off time of nearly 62 hours (3714 min). QC, quality control; qPCR, quantitative PCR; QCI-A, QIAGEN Clinical Insight Analyze; QCI-I, QCI-interpret.

GeneReader sequencing data analysis

The ATP assay was developed to focus only on clinically relevant mutations as included in approved therapeutics labels, major professional practice guidelines and active late-stage clinical trials. Thus, this approach results in a selection of genes and variants with an unparalleled level of direct clinical relevance. The integrated bioinformatics pipeline QCI-A allows a streamlined analysis of the sequences and identification of genetic aberrations, while providing intrinsic quality control measures to ensure confidence in calling of the variants. Of note, 16 of the 50 samples tested did not meet the industry standard 500× coverage threshold. Yet the GeneReader still successfully mapped the reads and correctly identified the variants, as summarised in table 2. In total, there were 56 mutations with clinical relevance positively identified (see online supplementary table S2), which showed an average and median hotspot coverage of around 5000× and 7650×, respectively (table 2).

Figure 2 Concordance between the in-house workflow using the MiSeq platform and the semiautomated GeneReader System. Direct allele frequency (AF) comparison between GeneReader and MiSeq. A high concordance ($R^2 = 0.946$) was achieved for 45 clinical variants.

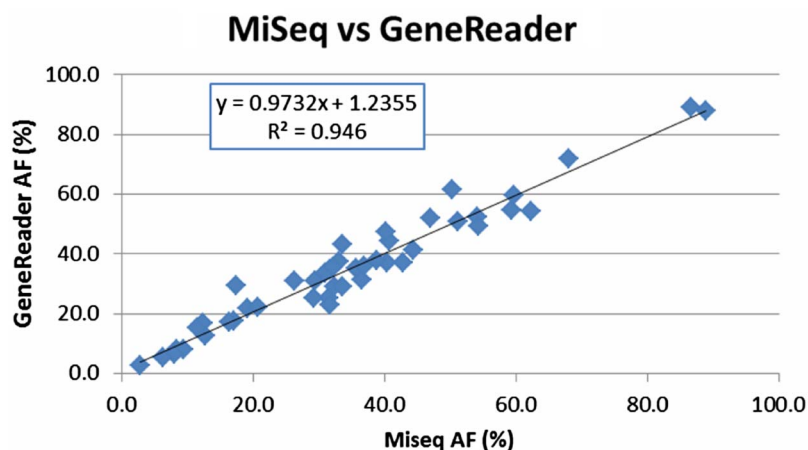

Confirmation of variants by MiSeq and Sanger sequencing

This study considered 50 clinical DNA samples processed by the routine diagnostics workflow of the laboratory for molecular pathology (Institute of Pathology at the University Hospital of Cologne). Hereby, we included samples from different origin (table 1), such as CRC, lung cancer, melanoma, GIST and gastric cancer. The samples also have been selected for their capacity to represent well-characterised variants with a clinical impact and to represent tumours with different tumour to normal cell ratios as shown in online supplementary table S2.

To ensure maximal sample consistency, the same DNA extractions were used for MiSeq or Sanger confirmation. Importantly, we observed a 100% agreement between GeneReader NGS system and the previously used MiSeq pipeline or the Sanger sequencing (see online supplementary table S2). For nine GIST samples with *PDGFRA* and *KIT* mutations (Q39–46), only Sanger sequencing confirmation data were available (see online supplementary table S2) with no direct variant allele frequency

Short report

information. For the remaining 45 samples, allele frequency mapping showed an extremely high degree of linear correlation ($R^2=0.946$) between the GeneReader System and the MiSeq pipeline (figure 2). Thus, importantly the concordance between the platforms is observed in a wide range of allele frequencies, from <5% to >90% (cf. figure 2).

Furthermore, we used the QCI-I software to assign clinical relevance and functional impact of these variants. This is a bioinformatics database built and continuously updated by a content curation team. This tool enables any laboratory to consider potential courses of action based on specific variants identified, by providing real-time information on approved or guideline-recommended therapeutics and active clinical trials. Such correct interpretation of tumour molecular changes is very important,⁸ in particular, because knowledge would otherwise be impractical for an individual laboratory to accumulate and update. For example, in addition to the well-known mutants in *BRAF* and *KRAS*, the activating p.Y772_A775 duplication in exon 20 of the *ERBB2* (*Her2*) gene was recognised in three samples. For this *ERBB2* (*Her2*) alteration, it was recently shown that patients with lung cancer, harbouring this mutation, benefit from treatment with *ERBB2* inhibitors, such as afatinib, neratinib, pelitinib and dacomitinib.^{9 10 11}

Take home messages

Targeted NGS by the semiautomatic workflow of the GeneReader System

- ▶ Proved a low hands-on time and
- ▶ Showed a high run performance and a high accuracy in mutation calling.

The integration of an automatic data transfer, analysis and interpretation,

- ▶ Ending by the report of the mutant with the potential pathogenic impact,
- ▶ Makes it as an easily accessible technology for molecular pathology laboratories.

Handling editor Runjan Chetty

Contributors UK and HA performed the GeneReader workflow, whereas CH, SM-B performed NGS by the conventional in-house workflow. CH, II and UK validated data by Sanger sequencing, and AF, RB and MO performed data interpretation and illustration. RHB, AF, YK, CH and MO wrote the manuscript, which was then reviewed by all authors.

Competing interests The University Hospital of Cologne, Institute of Pathology is in a collaboration agreement with Qiagen (Hilden, Germany). Reinhard H Büttner is on the Advisory Board of Qiagen. The authors declare no other conflict of interest. As of December 2016, the sequencing chemistry used in this study is not available in the USA.

Provenance and peer review Not commissioned; externally peer reviewed.

Open Access This is an Open Access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/4.0/>

REFERENCES

- 1 Horak P, Fröhling S, Glimm H. Integrating next-generation sequencing into clinical oncology: strategies, promises and pitfalls. *Esmo Open* 2016;1:e000094.
- 2 Houghton J, Hadd A, Zeigler R, et al. Integration of wet and dry bench processes optimizes targeted next-generation sequencing of low-quality and low-quantity tumor biopsies. *J Vis Exp* 2016;110:e53836.
- 3 Chen H, Luthra R, Goswami R, et al. Analysis of pre-analytic factors affecting the success of clinical next-generation sequencing of solid organ malignancies. *Cancers (Basel)* 2015;1699–715.
- 4 Grunewald I, Vollbrecht C, Meinrath J, et al. Targeted next generation sequencing of parotid gland cancer uncovers genetic heterogeneity. *Oncotarget* 2015;6:18224–37.
- 5 Heydt C, Fassunke J, Kunstlinger H, et al. Comparison of pre-analytical FFPE sample preparation methods and their impact on massively parallel sequencing in routine diagnostics. *PLoS ONE* 2014;9:e104566.
- 6 Knittel G, Liedgens P, Korovkina D, et al. B-cell-specific conditional expression of Myd88p.L252P leads to the development of diffuse large B-cell lymphoma in mice. *Blood* 2016;127:2732–41.
- 7 Vollbrecht C, Mairinger FD, Koitzsch U, et al. Comprehensive analysis of disease-related genes in chronic lymphocytic leukemia by multiplex PCR-based next generation sequencing. *PLoS ONE* 2015;10:e0129544.
- 8 Calabria I, Pedrola L, Berlanga P, et al. The new challenge in oncology: Next-generation sequencing and its application in precision medicine. *An Pediatr (Barc)* 2016;85:273.e1–e7.
- 9 Herter-Sprie G, Greulich H, and Wong KK. Activating mutations in *ERBB2* and their impact on diagnostics and treatment. *Front Oncol* 2013;3:86.
- 10 Li B, Lee A, Toole SO, et al. HER2 insertion YVMA mutant lung cancer: Long natural history and response to afatinib. *Lung Cancer* 2015;90:617–19.
- 11 Li B, Ross D, Aisner D, et al. HER2 amplification and HER2 mutation are distinct molecular targets in lung cancers. *J Thorac Oncol* 2016;11:414–19.



Use of the GeneReader NGS System in a clinical pathology laboratory: a comparative study

Ulrike Koitzsch, Carina Heydt, Hans Attig, Isabelle Immerschitt, Sabine Merkelbach-Bruse, Alessandro Fammartino, Reinhard H Büttner, Yi Kong and Margarete Odenthal

J Clin Pathol 2017 70: 725-728 originally published online April 11, 2017
doi: [10.1136/jclinpath-2017-204342](https://doi.org/10.1136/jclinpath-2017-204342)

Updated information and services can be found at:
<http://jcp.bmj.com/content/70/8/725>

These include:

- | | |
|-------------------------------|--|
| Supplementary Material | Supplementary material can be found at:
http://jcp.bmj.com/content/suppl/2017/04/11/jclinpath-2017-204342.DC1 |
| References | This article cites 10 articles, 2 of which you can access for free at:
http://jcp.bmj.com/content/70/8/725#ref-list-1 |
| Open Access | This is an Open Access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 4.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: http://creativecommons.org/licenses/by-nc/4.0/ |
| Email alerting service | Receive free email alerts when new articles cite this article. Sign up in the box at the top right corner of the online article. |

Topic Collections	Articles on similar topics can be found in the following collections Open access (127)
--------------------------	---

Notes

To request permissions go to:
<http://group.bmj.com/group/rights-licensing/permissions>

To order reprints go to:
<http://journals.bmj.com/cgi/reprintform>

To subscribe to BMJ go to:
<http://group.bmj.com/subscribe/>