
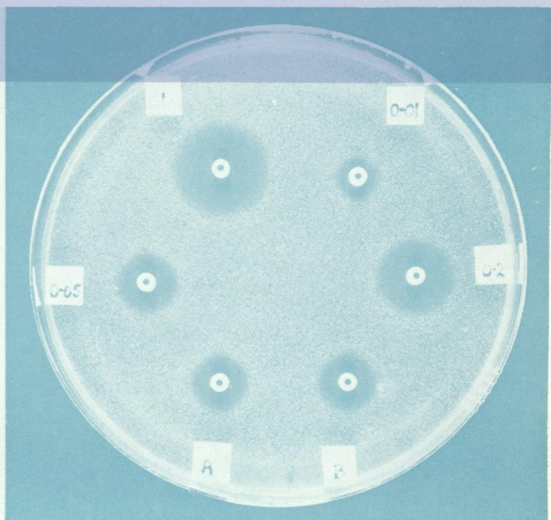
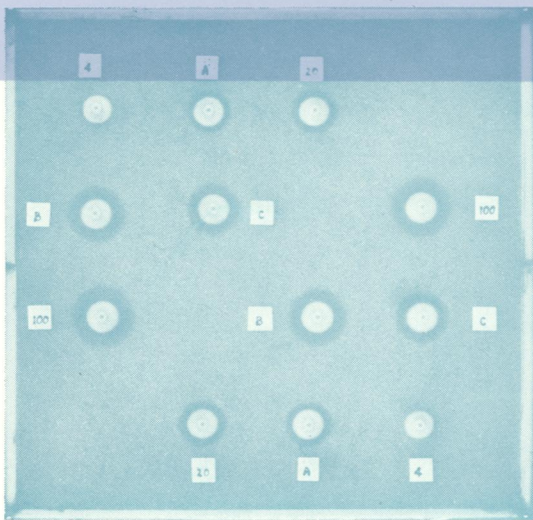


# Journal of Clinical Pathology

*The Journal of the Association of Clinical Pathologists*

Vol. 28, No. 10, October 1975

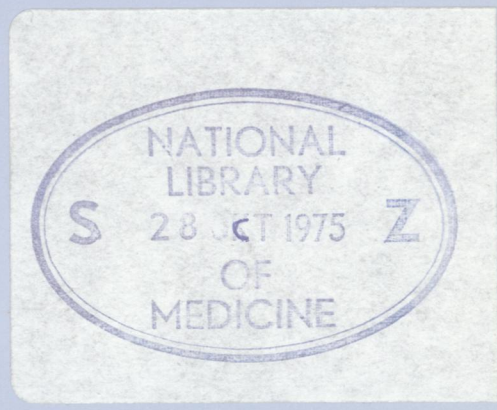

(Left) 5-fluorocytosine assay  
 Standards: 4, 20, 100  $\mu\text{g/ml}$  5-FC in serum  
 Test sera: A, B, C  
 Diagonal replication: C. pseudotropicalis

(Right) Clotrimazole assay  
 Standards: 0.01, 0.05, 0.2, 1.0  $\mu\text{g/ml}$  in serum  
 Test sera: A, B  
 C. pseudotropicalis. See figs 3 and 4, page 772.