

Colorimetric enzymatic measurement of serum total 3 α -hydroxy bile acid concentrations without extraction

MY QURESHI, SM SMITH, GM MURPHY

From the Gastroenterology Unit, 18th Floor, Guy's Tower, London Bridge, London SE1 9RT

SUMMARY A new method for the simpler colorimetric assay of serum total 3 α -hydroxy bile acid concentrations without prior extraction has been investigated. The lowest concentration that could be reliably measured was 3 μ mol/l and the results obtained were in agreement with those obtained using extraction and the spectrofluorimetric enzymatic assay ($y = 1.007x - 1.86$, $r = 0.99$, $n = 36$). Results for 20 normal sera collected after an overnight fast were 6.2 ± 5.1 μ mol/l (mean \pm SD) and in 20 normal plasma randomly collected were 4.9 ± 4.2 μ mol/l. This new assay is comparable in specificity and sensitivity to the older spectrofluorimetric enzymatic assays and convenient for routine use.

The measurement of serum bile acid concentrations has long been regarded by many authors as providing a very sensitive index of hepatobiliary function.¹⁻⁴ However, this test has yet to be accepted by clinical chemists and added to their routine assays for monitoring liver function. There are two reasons for this failure—lack of confidence in the specificity and sensitivity of serum bile acid measurements with regard to the detection of early liver disease^{5,6} and, of equal importance, lack of a method which fulfils the usual analytical reliability criteria and which could be readily applied in the clinical chemistry laboratory. This present report deals solely with the methodological problems and considers a possible solution in terms of an assay kit which has recently become commercially available.

The kit makes use of the following reactions:⁷



NADH + chromogen (NBT) $\xrightarrow{\text{Diaphorase}}$ Chromophore (Formazan) + NAD

The use of hydroxysteroid dehydrogenase for the determination of serum bile acid concentration is not new, normal values using spectrophotometry being first reported in 1964⁸ and those obtained with the more sensitive spectrofluorimetric assay in

1970.⁹ However, the linkage of the product NADH to a chromogen (nitrobluetetrazolium) to generate a chromophore provides a spectrophotometric end point with a sensitivity approaching that of the spectrophotometric assay but without the necessity of serum extraction. This direct and immediate assay thus represents a major advance in serum bile acid methodology.

Our primary concern therefore was to investigate the claims for this kit of sensitivity and specificity. To do this we largely followed a recommended scheme for the evaluation of kits in the clinical chemistry laboratory.¹⁰

Material and methods

NYCO-HSD-COL KIT METHOD

The kit was supplied by Nyegaard and Co, Oslo, Norway, and consisted of:

- (1) Sample reagent—which contains all the components necessary for the generation of the chromophore by bile acids and includes a serum inactivator,
- (2) Blank reagent—which contains all the constituents of the sample reagent with the exception of the hydroxysteroid dehydrogenase,
- (3) Sodium phosphate buffer, pH 7.0, 65 mmol/l (once reconstituted in this buffer, sample and blank reagents are stable for at least two weeks at 4°C),
- (4) Bile acid standard mixtures prepared in bile acid free bovine serum, of glycolate, glycodeoxy-

cholate and taurochenodeoxycholate, to final total bile acid concentrations of 10, 50 and 100 $\mu\text{mol/l}$, (5) Stop reagent—100 mmol/l HCl containing surfactant.

To perform the assay 500 μl of sample reagent reconstituted in the phosphate buffer was added to 200 μl each plasma and standard for the tests and for the blanks 500 μl blank reagent was used. After 10 min incubation at 37°C, 500 μl stop reagent was added to both test and blank tubes. The absorbance of each tube was read at 540 nm, a standard curve drawn, and results calculated in the usual way.

SPECTROFLUORIMETRIC ENZYMATIC ASSAY

This was performed as previously described⁹ with the modification that methanolic extracts of serum bile acids were prepared using Amberlite XAD-2 in the batch procedure.¹³

Results and discussion

SENSITIVITY

To examine the sensitivity of the proposed method analyses of doubling dilutions of the kit 50 $\mu\text{mol/l}$ standard were performed in duplicate on three occasions (Fig. 1). The range of absorbance obtained for each solution was small (coefficient of variation <2%) but it was not possible to distinguish between concentrations of $\leq 3.1 \mu\text{mol/l}$. The limit of detection of this method was therefore regarded as 3 $\mu\text{mol/l}$.

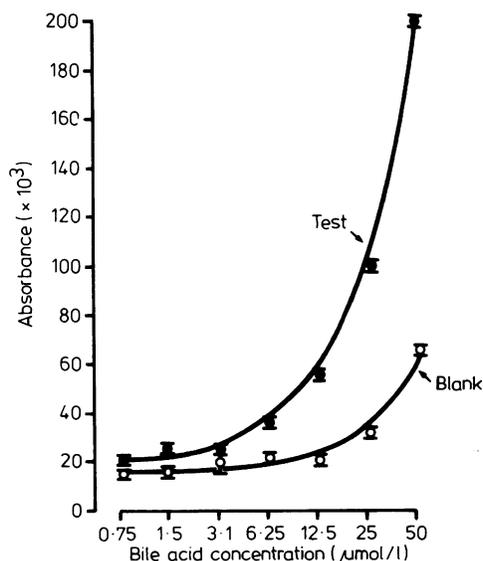


Fig. 1 Sensitivity. Absorbance (mean \pm SD) generated by dilutions of 50 $\mu\text{mol/l}$ standard solution.

Whereas this sensitivity is comparable with that of the original spectrofluorimetric enzymatic technique⁹ it is much less than any of the subsequent modifications.¹¹⁻¹⁹ It is unlikely, however, that the sensitivity of the new method will be shown to be inadequate in any clinical application. In particular, reductions in serum bile acid concentrations associated with gastrointestinal disease are more evident post-prandially than in the fasting state,^{20,21} and following meals total serum bile acid concentrations are normally above 3 $\mu\text{mol/l}$.^{3,4,12}

PRECISION

The "within-run" precision¹⁰ was estimated from the results of duplicate determinations on 37 different sera. The duplicate samples were randomly distributed throughout the run. For concentrations $\leq 10 \mu\text{mol/l}$, the coefficient of variation was 16% (7.2 ± 1.1 (mean \pm SD, $n = 20$)), for those 10–25 $\mu\text{mol/l}$ the CV was 10% (14.6 ± 1.5 ; $n = 9$), and for those $>25 \mu\text{mol/l}$ the CV was 6.8% (63.1 ± 4.3 ; $n = 8$).

The "between-day" precision¹⁰ was estimated from the results obtained on three sera each analysed in duplicate on 17 consecutive days. The CV at $<10 \mu\text{mol/l}$ was 12% (5.8 ± 0.7), between 11–25 $\mu\text{mol/l}$ the CV was 10% (31.7 ± 3.2), and at $>25 \mu\text{mol/l}$ the CV was 2% (105 ± 2.1).

Analysis of the "control" serum supplied with the kit gave results with CV of 9% (39.9 ± 3.6).

SERUM INTERFERENCE

In order to evaluate possible interference in this assay from serum constituents other than bile acids, the following experiments were performed. Two sera were diluted with isotonic saline, and the dilutions analysed using the kit. The results obtained on each of the dilutions were expressed as a percentage of the concentration found in the corresponding undiluted serum. Whilst the results for undiluted, 1/2 and 1/4 dilutions were linear and parallel to the standard curve, recoveries from the 1/8 dilution were poor (Table). To investigate this further, standard solutions of taurocholic acid were prepared in water and in serum. Although both sets of results were linear, parallelism with the standard curve was only found in the presence of serum (Fig. 2). It was concluded that there is in serum a factor which enhances the reaction and that if the method is to be applied to unextracted sera, the dilutions of sera must be less than 1/4. (This caution may be particularly relevant to analyses of bile and bile-rich duodenal contents with this kit and aqueous solutions of standards of appropriate concentrations should be used—Barbara H Billing, personal communication 1983.)

Effect of dilution in isotonic saline

Dilution	Serum no	
	1	2
Neat	57.6 μ mol	160 μ mol
1/2	103%	99%
1/4	102%	99%
1/8	55%	88%

COMPARISON WITH THE ENZYMATIC FLUORIMETRIC METHOD

The results obtained using the spectrophotometric assay kit were compared with those obtained on the same samples using the enzymatic fluorimetric assay.⁹ For that procedure, bile acids were extracted from serum using Amberlite XAD-2 using the batch procedure and the fluorimetric assay applied to the methanolic extracts with little modification from the method originally described.⁹ Samples which were haemolysed or which had become turbid on storage at -20°C were excluded from this study. The results obtained using the kit were usually lower than those obtained on the same sample using the spectrofluorimetric assay and the two sets of data were far from identical. The correlation, however, between the results of the two methods was satisfactory (Fig. 3).

NORMAL VALUES

Results in sera obtained from 20 laboratory staff who had fasted overnight were 6.2 \pm 5.1 μ mol/l (mean \pm SD; range 3-16.3 μ mol/l). Results in plasma (sodium citrate), randomly collected in relation to meal times, from staff who were acting as controls in another investigation were 4.9 \pm 4.2 (mean \pm SD; range 3-15.1 μ mol/l). There is some disagreement in the literature concerning the normal range of serum bile acid concentrations using enzymatic fluorimetric techniques. Some groups report normal ranges similar to those obtained by

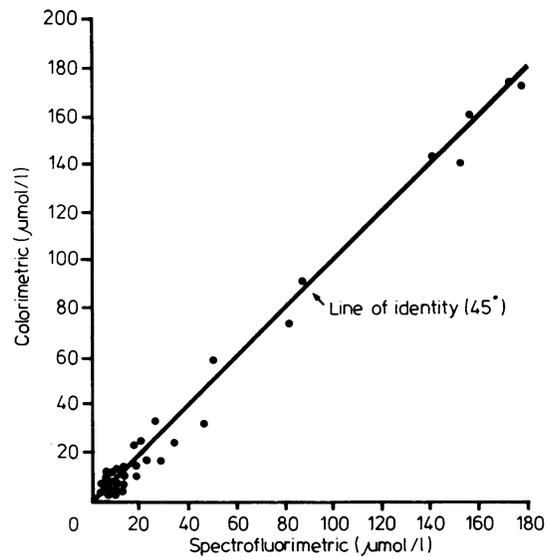


Fig. 3 Serum total bile acid concentrations (μ mol/l). Colorimetric v spectrofluorimetric assay ($y = 1.007x - 1.86, r = 0.993$).

the present spectrophotometric technique in apparently fasting subjects;^{13 22 23} others find these higher values only in non-fasting subjects.^{4 14 24} Perhaps the real difficulty lies in assuming that no contraction of the gallbladder or movement of the bile acid pool occurs during fasting.

Of all the methods (enzymatic, radioimmunoassay, gas chromatography, gas chromatography-mass spectrometry, high pressure liquid chromatography-mass spectrometry) currently used to measure serum bile acid concentration, the enzymatic method is the least time consuming, complicated and expensive. Our conclusion is that this colorimetric enzymatic method for serum total

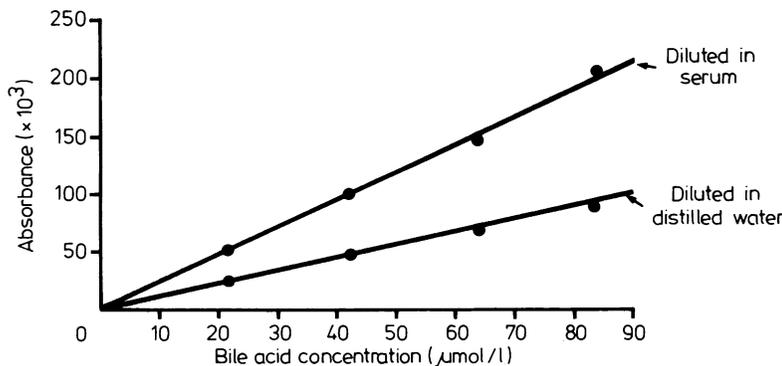


Fig. 2 Standard solutions. Absorbance generated by standard solutions of taurocholate prepared in either water or serum as described in text.

bile acid measurement is comparable to the older fluorimetric enzymatic assays in specificity and more suitable for routine use.

The authors thank Prof DN Baron and Prof BH Billing for their helpful criticism of this manuscript. GMM is a Wellcome Trust Senior Lecturer.

References

- ¹ Kaplowitz N, Kok E, Javitt NB. Postprandial serum bile acid for the detection of hepatobiliary disease. *JAMA* 1973;**225**:292-3.
- ² Korman MG, Hofman AF, Summerskill WHJ. Assessment of activity of chronic liver disease. Serum bile acids compared with conventional tests and histology. *N Engl J Med* 1974;**290**:1399-1402.
- ³ Barnes S, Gallo GA, Trash DB, Morris JS. Diagnostic value of serum bile acid estimations in liver disease. *J Clin Pathol* 1975;**28**:506-9.
- ⁴ Kobayashi K, Allen RM, Bloomer JR, Klatskin G. Enzymatic fluorometry for estimating serum bile acid concentrations. *JAMA* 1979;**241**:2043-5.
- ⁵ Isaacs PET, Murphy GM, Matthews LM, Sampson D, Dowling RH. Serum bile acid concentration in gastrointestinal disease. *Clin Sci* 1979;**56**:29p.
- ⁶ Samuelson K, Aly A, Johansson C, Norman A. Evaluation of fasting serum bile acid concentration in patients with liver and gastrointestinal disorders. *Scand J Gastroenterol* 1981;**16**:225-34.
- ⁷ Mashige F, Imai K, Osuga T. A simple and sensitive assay of total serum bile acids. *Clin Chim Acta* 1976;**70**:79-86.
- ⁸ Iwata T, Yamasaki K. Enzymatic determination and thin-layer chromatography of bile acids in blood. *J Biochem (Tokyo)* 1964;**56**:394-424.
- ⁹ Murphy GM, Billing Barbara H, Baron DN. A fluorimetric and enzymatic method for the estimation of serum bile acids. *J Clin Pathol* 1970;**23**:594-8.
- ¹⁰ Percy-Robb IW, Broughton PMG, Jennings RD, et al. A recommended scheme for the evaluation of kits in the clinical chemistry laboratory. *Ann Clin Biochem* 1980;**17**:217-26.
- ¹¹ Schwarz HP, Bergmann KV, Paumgartner G. A simple method for the estimation of bile acids in serum. *Clin Chim Acta* 1974;**50**:197-206.
- ¹² Fausa O. Quantitative determination of serum bile acids using a purified 3 α -hydroxysteroid dehydrogenase. *Scand J Gastroenterol* 1975;**10**:747-52.
- ¹³ Barnes S, Chitranukroh A. A simplified procedure for the isolation of bile acids from serum based on batch extraction with the non-ionic resin - Amberlite XAD-7. *Ann Clin Biochem* 1977;**14**:235-9.
- ¹⁴ Siskos PA, Cahill PT, Javitt NB. Serum bile acid analysis: a rapid, direct enzymatic method using dual-beam spectrofluorimetry. *J Lipid Res* 1977;**18**:666-71.
- ¹⁵ Mashige F, Osuga T, Tanake N, Imai K, Yamanaka M. Continuous flow determination of bile acids in serum and its clinical application. *Clin Chem* 1978;**24**:1150-4.
- ¹⁶ Brussgaard A, Pederson LR, Sorenson H. Determination of total 3 α -hydroxy bile acids in serum. *Clin Chim Acta* 1979;**93**:1-8.
- ¹⁷ Barnes S, Spenny JG. Improved enzymatic assays for bile acids using resazurin and NADH oxidoreductase activity from *Clostridium kluyveri*. *Clin Chim Acta* 1980;**102**:241-5.
- ¹⁸ Starkey BJ, Marks V. Determination of total bile acids in serum. A comparison of a radioimmunoassay with an enzymatic-fluorimetric method. *Clin Chim Acta* 1982;**119**:165-77.
- ¹⁹ Roda A, Kruka LJ, DeLuca M, Hofmann AF. Bioluminescence measurement of primary bile acids using immobilized 7 α -hydroxysteroid dehydrogenase: application to serum bile acids. *J Lipid Res* 1983;**23**:1354-61.
- ²⁰ Russo NF, Korman MG, Hoffman NE, et al. Dynamics of the enterohepatic circulation of bile acids; postprandial serum concentration of conjugates of cholic acid in health, cholecystectomized patients and patients with bile acid malabsorption. *New Engl J Med* 1974;**291**:689-92.
- ²¹ Suchy FS, Ballistreri WF. Ileal dysfunction in Crohn's disease assessed by the postprandial serum bile acid response. *Gut* 1981;**22**:948-52.
- ²² Thjodleifsson B, Barnes S, Chitranukroh A, Billing B, Sherlock S. An assessment of the plasma disappearance of cholesteryl-1-¹⁴C-glycine. As a test of hepatobiliary disfunction. *Gut* 1977;**18**:697-702.
- ²³ Pare P, Hoeffs JC, Aschcavi M. Determinants of serum bile acids in chronic liver disease. *Gastroenterology* 1981;**81**:959-64.
- ²⁴ Ferraris R, Colombatti G, Florentine MT, Carosso R, Arossa W, De La Pierre M. Diagnostic value of serum bile acids and routine liver function tests in hepatobiliary diseases. *Dig Dis Sci* 1983;**28**:129-35.

Requests for reprints to: Dr GM Murphy, Gastroenterology Unit, 18th Floor, Guy's Tower, London Bridge, London SE1 9RT, England.