

Choosing wisely during the COVID-19 pandemic: optimising outpatient cancer care while conserving resources with a new algorithm to report automated ANC results

In the face of the COVID-19 pandemic, efficient outpatient management is paramount to minimise wait times and reduce exposure to respiratory illnesses, particularly in patients with cancer receiving chemotherapy. The complete blood cell count (CBC) with white cell count (WCC) differential (CBC-D) is an essential laboratory test used to screen cancer patients prior to chemotherapy. Patients receiving cytotoxic chemotherapy are at risk for developing neutropenia; the absolute neutrophil count (ANC) can be used to determine if a patient is neutropenic.¹ Neutropenia is generally defined as an ANC $<1.5 \times 10^9/L$ – $2.0 \times 10^9/L$, with severe neutropenia defined as $<0.5 \times 10^9/L$.²

WCC differential analysis is performed by automated haematology platforms in the clinical laboratory. These platforms have been found to provide accurate and precise ANC results.³ However, automated results often require manual review if the analysis is associated with instrument flags that indicate the potential for inaccurate results. Review and confirmation of flagged results by laboratory technologists is time consuming and increases test result

Table 1 Distribution of differential flags requiring manual peripheral blood smear review

Instrument flags	No of flagged instances	
	Solid tumour malignancies, %	Haematological malignancies, %
Nucleated red blood cells (NRBC)	512 (33)	256 (20)
Blasts/abnormal lymphoid	386 (25)	297 (23)
Monocytosis ($\geq 1.5 \times 10^3/\mu L$ or $\geq 30\%$)	106 (7)	167 (13)
Immature granulocytes	189 (12)	137 (11)
WCC abnormal scattergram	123 (8)	112 (9)
Atypical lymphoid	127 (8)	51 (4)
Previous sample with blasts	65 (4)	167 (13)
Eosinophilia ($\geq 20\%$)	35 (2)	10 (0.8)
Absolute lymphocytosis ($\geq 5 \times 10^3/\mu L$)	25 (2)	93 (7)
Basophilia ($\geq 1 \times 10^3/\mu L$ or $\geq 5\%$)	4 (0.3)	9 (0.7)
New patient with WCC $> 11 \times 10^9/L$	1 (0.1)	1 (0.1)
Total flags	1573	1300

WCC, white cell count.

turnaround time (TAT), thereby prolongs onset of chemotherapy.^{4–7} Given that chemotherapy administration requires an adequate ANC, we examined the reliability of the automated ANC in the presence of instrument flags in outpatients with solid tumour and haematological malignancies. We aimed to confirm if discrete ordering of a ‘CBC with ANC only’ test could be used to replace the traditional CBC with full WCC differential (CBC-D) and shorten patient wait times.

We performed a retrospective analysis of 1648 sequential CBC with WCC differential results flagged for manual peripheral blood smear review performed for patients with cancer. Results across five outpatient locations were analysed during October 2018. The cases were separated based on malignancy type, solid tumour (n=1078) or haematological malignancies (n=570). The accuracy of automated ANC results

(Sysmex XN) was assessed by comparison to the manual differential using Rumke statistics.⁸ Manual review of automated differential results was performed by experienced clinical laboratory technologists and consisted of either a peripheral blood smear review with confirmation of automated differential results or a full 100 cell manual differential.

Differential review flags associated with automated CBC-D results are summarised in table 1. Multiple flags were frequently observed in the same sample. As shown in figure 1, the automated differential was confirmed by peripheral blood smear review in 327 of 1078 (30%) samples from patients with solid tumour malignancies. A full manual differential was performed in the remaining 751 of 1078 cases (70%). In contrast, the automated differential was confirmed by peripheral blood smear review in 108 of 570 (19%) samples from

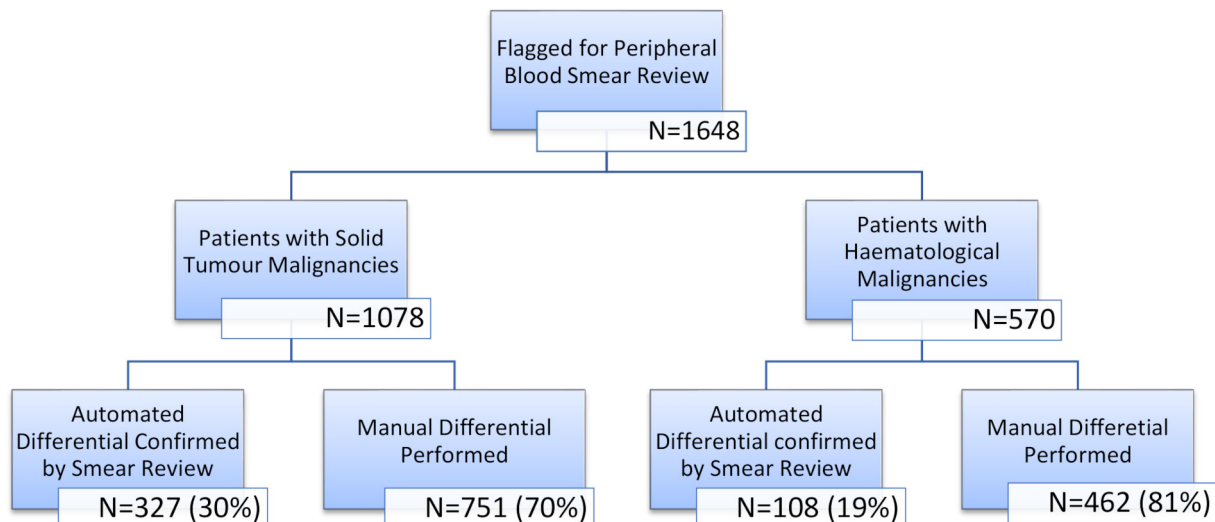


Figure 1 Study design to evaluate automated ANC performance in flagged CBC-D samples. ANC, absolute neutrophil count; CBC-D, complete blood cell count differential.

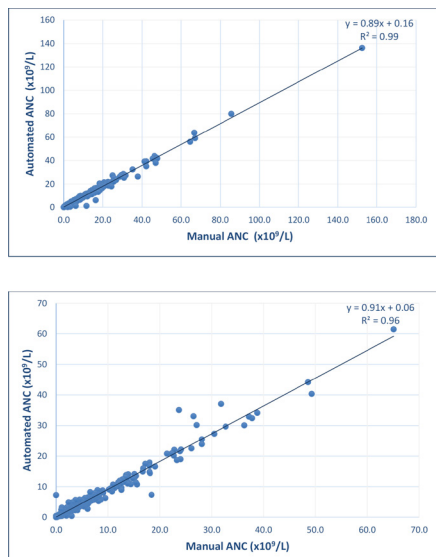


Figure 2 Correlation between manual and flagged automated ANC results in patients with solid tumour malignancies (top) and in patients with haematological malignancies (bottom). ANC, absolute neutrophil count.

patients with haematological malignancies, and a full manual differential was performed in the remaining 462 of 570 cases (81%). The correlation between manual and automated ANC results was strong for patients with solid tumour and those with haematological malignancies with a R^2 of 0.99 (slope=0.89) and a R^2 of 0.96 (slope=0.91), respectively, despite instrument flags (figure 2). Subset analysis of haematological malignancies showed a similarly strong correlation between automated and manual ANC results for samples from patients with leukaemia, lymphoma, plasma cell dyscrasia, bone marrow transplant (BMT), myelodysplastic syndrome (MDS), myeloproliferative neoplasm (MPN) and non-malignant haematological disorders (table 2).

Discordant automated and manual neutrophil results were identified in a total of 247 cases; 102 from patients with solid

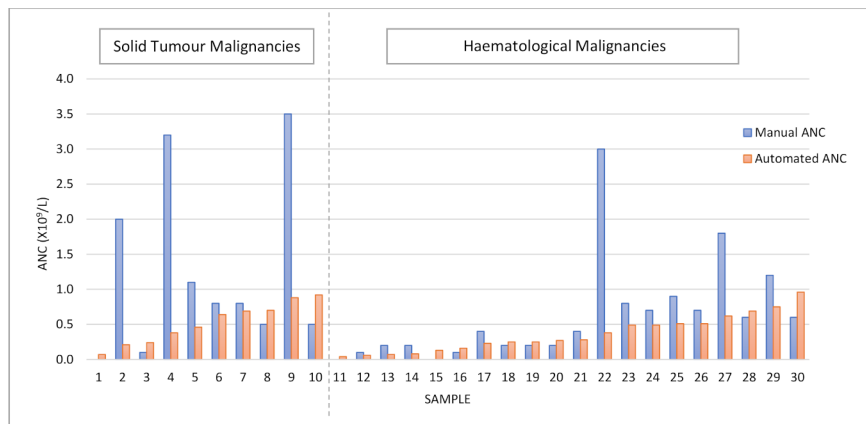


Figure 3 Differences between flagged automated and manual ANC results for samples with an automated ANC $\leq 1000/\mu\text{L}$ in patients with solid tumour (n=10) and in haematological (n=20) malignancies. ANC, absolute neutrophil count.

tumour malignancies and the remaining 145 from patients with haematological malignancies. The majority of these cases (n=217), had an automated ANC $> 1.0 \times 10^9/\text{L}$, and the difference in ANC results was not clinically significant. In general, automated ANC results were slightly lower than manual results. Thirty samples, 10 from patients with solid tumours and 20 from patients with haematological malignancies, were found to have discordant ANC results with an automated ANC of $\leq 1.0 \times 10^9/\text{L}$ (figure 3).

This study investigated the feasibility of reporting a CBC with ANC only in cancer patients with solid tumour or haematological malignancies. The data support creating a distinct test order for ‘CBC with ANC only,’ when the ANC is required for the initiation of chemotherapy, discharge or other intervention. Our results confirm previous reports describing the validity of the automated ANC in a general patient population^{3,5-7} and that the automated ANC results are consistently marginally lower than the manual count.⁹ Additionally, this study provides new data on patients with haematological malignancies, subclassifying haematological malignancy by type (leukaemia, lymphoma, MDS, MPN and plasma cell dyscrasias), as

well as including patients with recent BMT. Based on our review of discordant manual and automated ANC results, as well as the clinical definition of neutropenia, we suggest manual review of samples with flagged automated differential results, when the ANC is $< 1.0 \times 10^9/\text{L}$.

A ‘CBC with ANC only’ order has the potential to decrease the manual review of CBC with differentials in patients with solid tumour and haematological malignancies by 91% and 75%, respectively (table 3). If clinicians transition from ordering a conventional CBC with differential to the ‘CBC with ANC only’ test option patient wait times can be reduced and laboratory and clinical resources conserved. In our institution, the TAT for a CBC with automated ANC is 10–15 min compared with 30–60 min for a manual ANC. A reduction in manual peripheral blood smear reviews from 1648 to 247 would represent substantial laboratory labour savings. Additional institutional savings are expected based on more efficient management of patient appointments and discharge.

The need for more efficient patient management is highlighted during the COVID-19 pandemic. Reduction in staffing

Table 2 ANC correlation in samples from patients with haematological malignancies

Haematological malignancy type	Total cases, %	ANC confirmed by smear review, %	Manual differential performed, %	Automated and manual differential correlation characteristics	
				R^2	Slope
Lymphoma	196 (34)	35 (6)	161 (28)	0.97	0.85
Leukaemia	189 (33)	18 (3)	171 (30)	0.95	0.99
Plasma cell dyscrasia*	59 (10)	21 (3)	38 (6)	0.97	0.84
BMT	56 (10)	15 (3)	41 (7)	0.97	0.85
MDS	38 (6)	13 (2)	25 (4)	0.99	0.89
MPN	25 (4)	6 (1)	19 (3)	0.99	0.94
Non-malignant haematological disorders	7 (1)	0 (0)	7 (100)	0.98	0.88

*Plasma cell dyscrasias include multiple myeloma and plasmacytoma.


ANC, absolute neutrophil count; BMT, bone marrow transplant; MDS, myelodysplastic syndrome; MPN, myeloproliferative neoplasm.

Table 3 Proposed reduction in automated ANC review of flagged CBC-D samples

	Solid tumour malignancies (N)	Haematological malignancies (N)
Current state: manual review of all flagged samples	1078	570
Proposed manual review for flagged samples with automated ANC $\leq 1000/\mu\text{L}$	102	145
Anticipated reduction in manual review for automated ANC in flagged samples	91%	75%

ANC, absolute neutrophil count; CBC-D, complete blood cell count differential.

and the necessity for social distancing in the clinical laboratory as well as patient care areas has led healthcare institutions to reconsider established workflows. A 'CBC with ANC only' test offers an opportunity to preserve resources without adversely impacting patient care.

Maly Fenelus , **Tamiqua Graham, Ryan Golden, Jessica L Bautista, Rachel J So, Nora Plante, Ellinor I B Peerschke**

Laboratory Medicine, Memorial Sloan Kettering Cancer Center, New York city, New York, USA

Correspondence to Dr Maly Fenelus, Laboratory Medicine, Memorial Sloan Kettering Cancer Center, New York, NY 10065, USA; fenelusm@mskcc.org

Handling editor Mary Frances McMullin.

Contributors MF and EIBP designed the research, analysed data and wrote the paper. TG, RG, RJS and MF performed research. RJS, NP and JLB analysed data.

Funding This study was funded in part by National Cancer Institute (Cancer Center Support, grant P30 CA008748).

Competing interests None declared.

Patient consent for publication Not required.

Provenance and peer review Not commissioned; internally peer reviewed.

This article is made freely available for use in accordance with BMJ's website terms and conditions for the duration of the covid-19 pandemic or until otherwise determined by BMJ. You may use, download and print the article for any lawful, non-commercial purpose (including text and data mining) provided that all copyright notices and trade marks are retained.

© Author(s) (or their employer(s)) 2021. No commercial re-use. See rights and permissions. Published by BMJ.



To cite Fenelus M, Graham T, Golden R, *et al.* *J Clin Pathol* 2021;**74**:202–204.

Received 15 September 2020

Revised 26 October 2020

Accepted 27 October 2020

Published Online First 16 November 2020

J Clin Pathol 2021;**74**:202–204.

doi:10.1136/jclinpath-2020-207114

ORCID iD

Maly Fenelus <http://orcid.org/0000-0003-1959-4489>

REFERENCES

1 Yang B-B, Savin MA, Green M. Prevention of chemotherapy-induced neutropenia with pegfilgrastim: pharmacokinetics and patient outcomes. *Chemotherapy* 2012;**58**:387–98.

- McPherson RA, Pincus MR. *Henry JB. Henry's clinical diagnosis and management by laboratory methods*. Philadelphia: Saunders Elsevier, 2011.
- Amundsen EK, Urdal P, Hagev T-A, *et al.* Absolute neutrophil counts from automated hematology instruments are accurate and precise even at very low levels. *Am J Clin Pathol* 2012;**137**:862–9.
- Jatoi A, Jaromin R, Jennings L, *et al.* Using the absolute neutrophil count as a stand-alone test in a hematology/oncology clinic: an abbreviated test can be preferable. *Clin Lab Manage Rev* 1998;**12**:256–60.
- Sireci AN, Herlitz L, Lee K, *et al.* Validation and implementation of an algorithm for reporting the automated absolute neutrophil count from selected flagged specimens. *Am J Clin Pathol* 2010;**134**:720–5.
- Friis-Hansen L, Saelsen L, Abildstrøm SZ, *et al.* An algorithm for applying flagged Sysmex XE-2100 absolute neutrophil counts in clinical practice. *Eur J Haematol* 2008;**81**:140–53.
- Stephens L, Hintz-Prunty W, Bengtsson H, *et al.* Impact of integrating Rumke statistics to assist with choosing between automated hematology analyzer differentials vs manual differentials. *JALM* 2017.
- Rumke C. The statistically expected variability in differential counting. In: Koepke J, ed. *Cap conference*. Aspen, CO: College of American Pathologists, 1977: 1978. 39–45.
- Ruzicka K, Veitl M, Thalhammer-Scherrer R, *et al.* The new hematology analyzer Sysmex XE-2100: performance evaluation of a novel white blood cell differential technology. *Arch Pathol Lab Med* 2001;**125**:391–6.